

FLUKE®

789/787B ProcessMeter™

Quick Reference Guide


⚠ Warning

To prevent possible electrical shock, fire, or personal injury, read the “789/787B Safety Information” before you use this Product.


📖 Consult user documentation.

Go to www.fluke.com to register your product and find more information.


~ V ~ V ~ mV

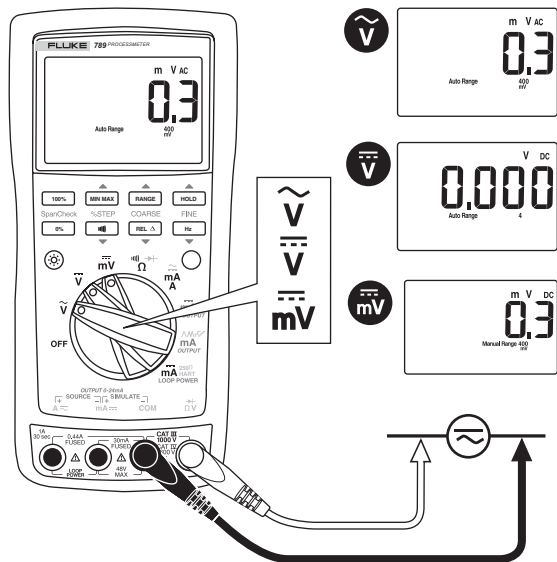


Ω

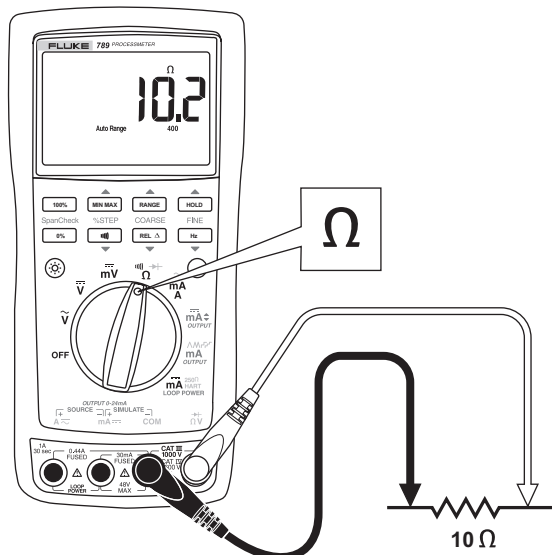


)))

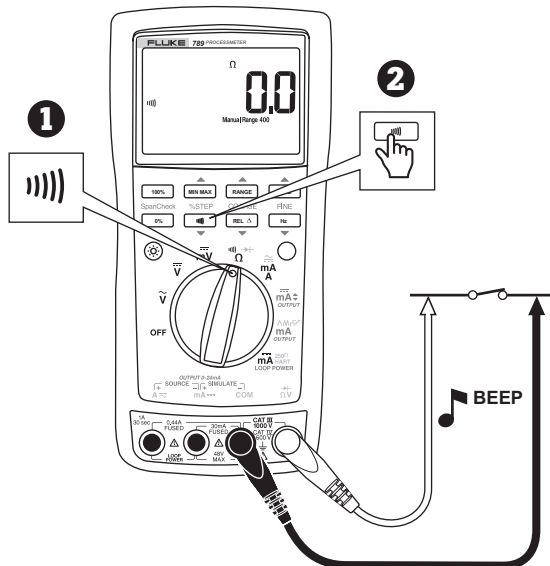



mA/A

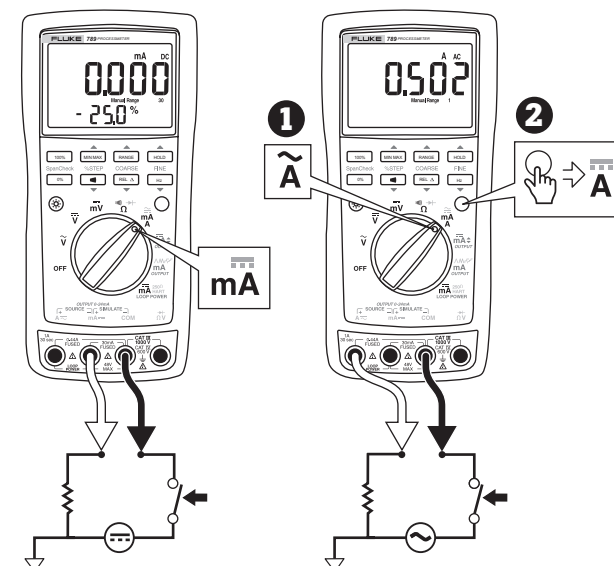


Measurement MIN MAX

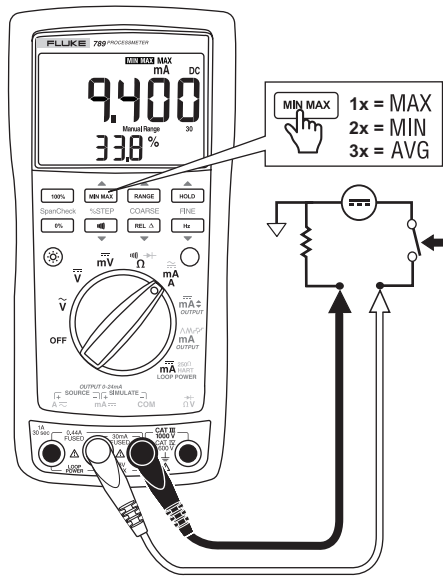

Fuse

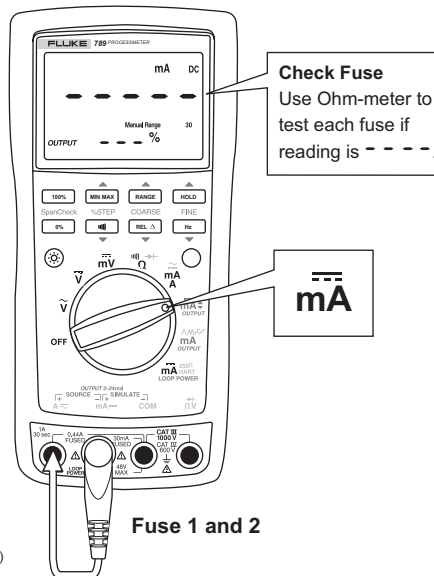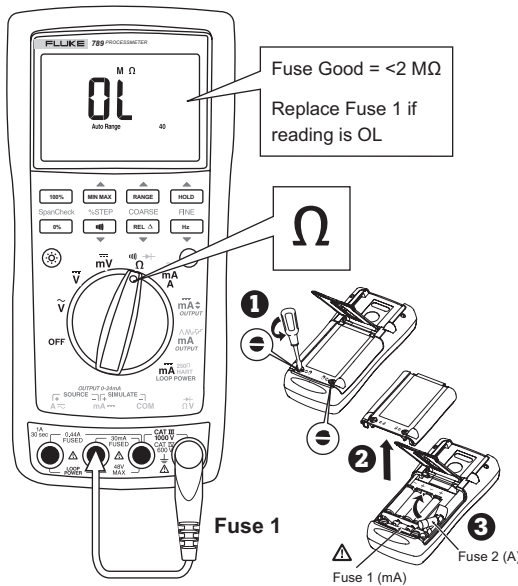


4 x AA Alkaline

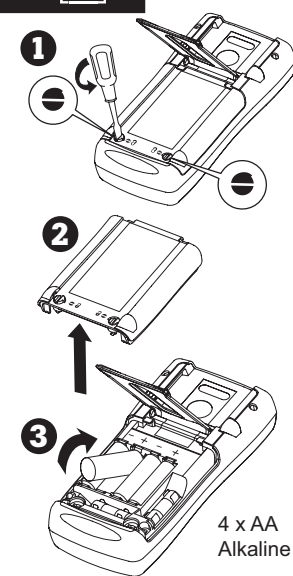





Good Diode

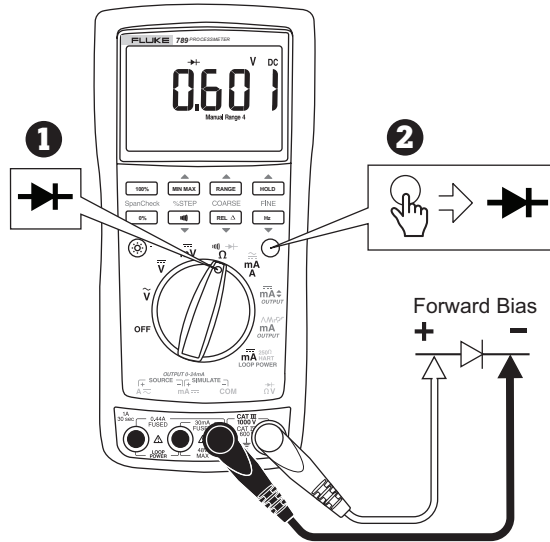


Good Diode

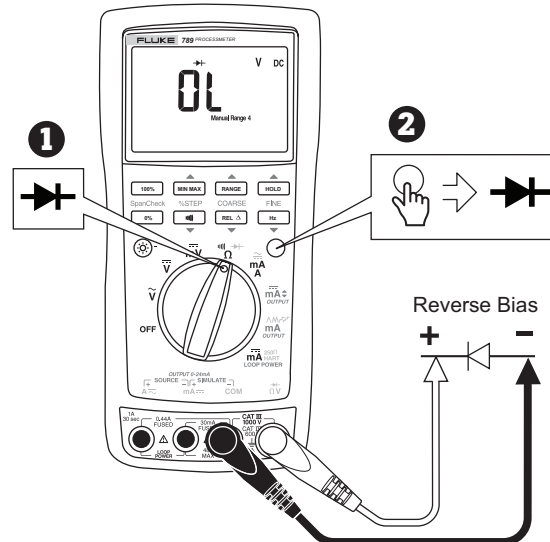


Bad Diode

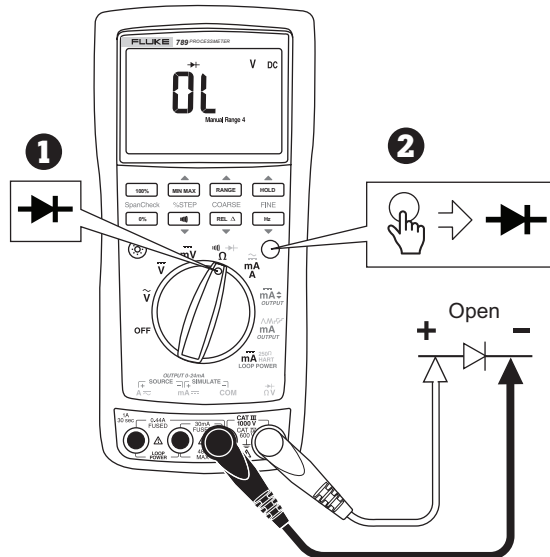


Bad Diode

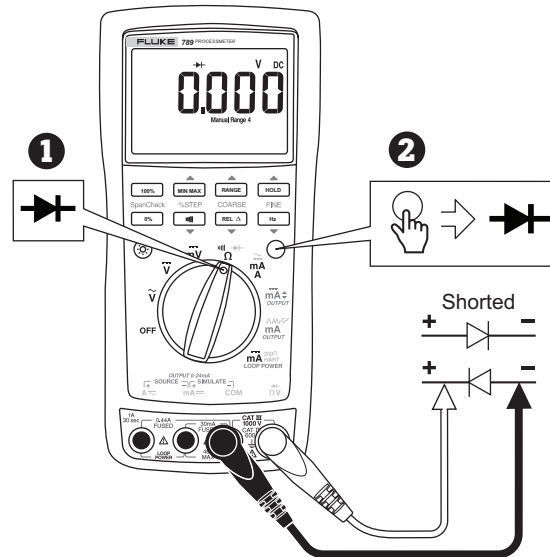


Output Source

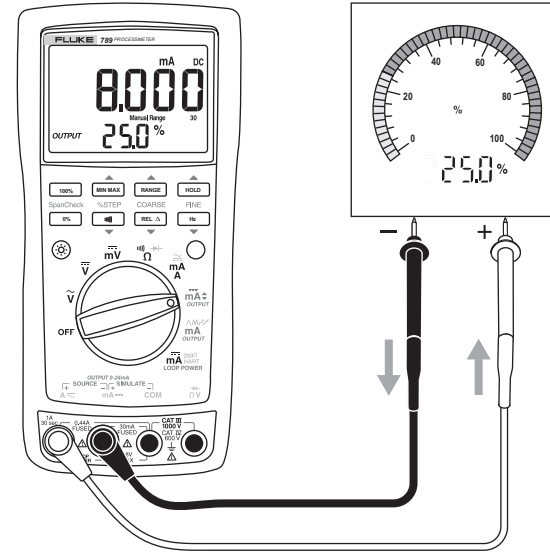

Output Simulate

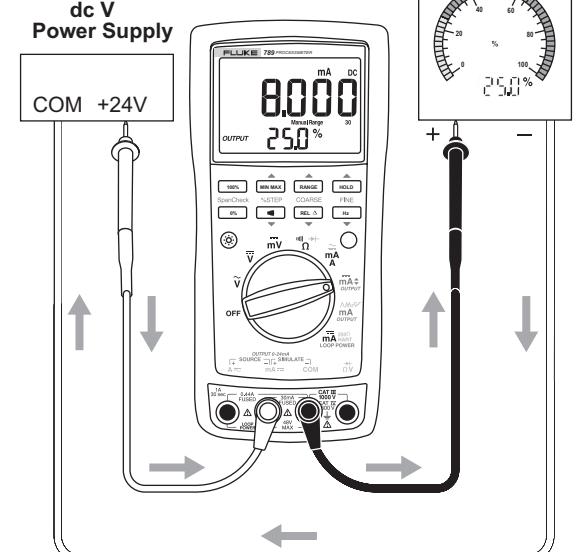

Supplying Loop Power (789 only)

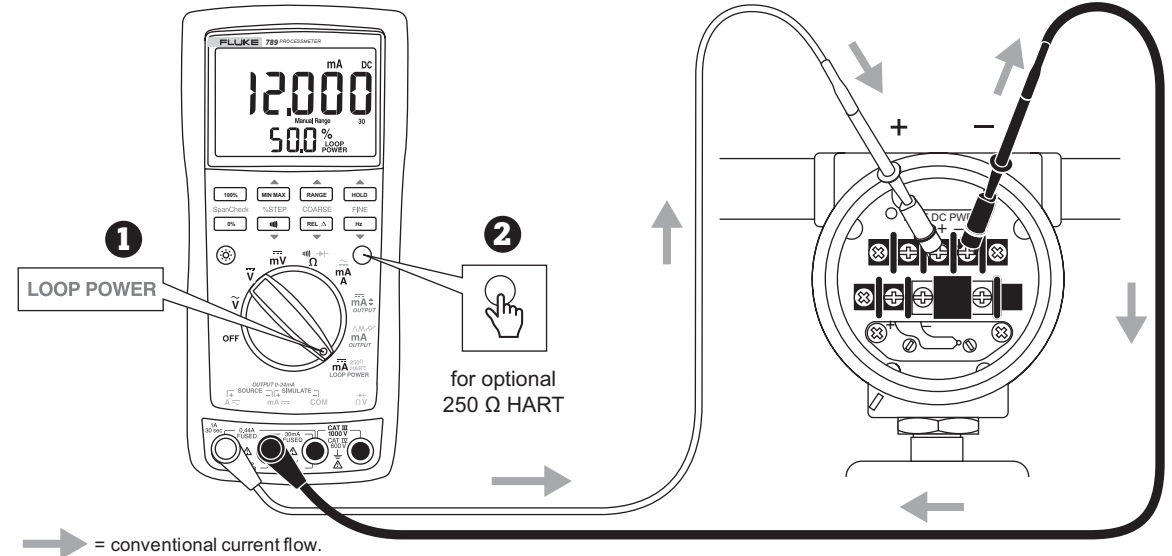

→ = conventional current flow.